SPECIFICATIONS

PARTICLE SENSOR

KS-16F



3-20-41 Higashimotomachi, Kokubunji, Tokyo 185-8533, Japan

Outline

The KS-16F is designed to be used as an in-line sensor in a system for measuring the size and number of particles in liquid, using the light-scattering method. Sample fluid contacting parts are made of sapphire and PFA, allowing direct measurement of hydrofluoric acid solutions. Measurement results are output via a built-in interface. The KS-16F consists of the sensor unit and the power supply unit. Particles are measured in five size ranges ($\geq 0.1 \mu m$, $\geq 0.15 \mu m$, $\geq 0.3 \mu m$, $\geq 0.5 \mu m$), and the sample flow rate is 10 mL per minute.

The KS-16F does not have measurement controls or a display for measurement results. It is designed to be used under control of external equipment such as a computer, and to send measurement results to the external equipment. A standard serial interface and a special Rion multi-point interface for multi-point measurements are built in.

As the KS-16F does not incorporate a flow control circuit for the sample fluid, the flow rate of the sample fluid must be controlled by external means.

* All company names and product names mentioned in this specifications are trademarks or registered trademarks of their respective owners.

Specifications


| Optical system | 90° sideway light-scattering method | | |
|--|--|--|--|
| Light source | Laser diode (rated output 200 mW; wavelength 830 nm) | | |
| Laser product class | Class 1, IEC 60825-1:2014 | | |
| | Internal particle detection mechanism uses Class 3B laser | | |
| Light detector | PIN type photodiodes | | |
| Materials of parts exposed to sample fluid | | | |
| | Sapphire, PFA | | |
| Allowable sample fluid types | | | |
| | Fluids which do not corrode the fluid contact materials | | |
| Calibration | Polystyrene latex (PSL) spheres with refractive index 1.6 in pure | | |
| | water | | |
| Minimum detectable particle size | | | |
| | 0.1 μm | | |
| Measurable particle size range | | | |
| | 0.1 μm to 2 μm | | |
| | (with PSL particles of refractive index 1.6 in pure water) | | |
| Measurement size range | Five channels($\geq 0.1 \ \mu m$, $\geq 0.15 \ \mu m$, $\geq 0.2 \ \mu m$, $\geq 0.3 \ \mu m$, $\geq 0.5 \ \mu m$) | | |


| Counting efficiency | $60\% \pm 15\%$ (when measuring PSL particles with about 0.3 µm diameter at a range setting of 0.2 µm or higher with the value shown on the reference instrument) | | | |
|---|--|--|--|--|
| Sample flow rate | 10 mL/min | | | |
| Maximum particle number concentration 1200 particles/mL (coincidence loss 5% for 0.1 µm particles) | | | | |
| Sample fluid temperature range +15°C to +35°C (no moisture condensation on flow cell) | | | | |
| Allowable sample fluid pressure 300 kPa or less (gauge reading) | | | | |
| Warm-up time | 10 minutes | | | |
| Sample fluid ports | | | | |
| INLET: OUTLET: PURGE: | Sample fluid inlet, 2 mm × 4 mm dia. flared tube joint Sample fluid outlet, 2 mm × 4 mm dia. flared tube joint Purge gas inlet, Rc 1/8 (1/8 PT female) | | | |
| Indicators | | | | |
| CELL | | | | |
| Lit (green): | Particle sensor (flow cell) is operating normally. | | | |
| Lit (red): | Particle sensor is not operating normally, due to contamination, condensation or other causes, or particle concentration in sample fluid exceeds maximum rating of unit. | | | |
| Off: | Light source is turned off. | | | |
| LD | | | | |
| Lit (green): | Light source (laser diode) is operating normally. | | | |
| Lit (red): | Light source has exceeded rated temperature range. | | | |
| Flashing (red): | Light source error other than temperature error has occurred. | | | |
| Off: | Light source is turned off. | | | |
| POWER | Lights up when power to the unit is turned on. | | | |
| Input/output connectors | | | | |
| SERIAL: | Serial interface (D-sub, 9-pin) | | | |
| DATA LINK: ALARM (1, 2): | Interface for configuring a multi-point monitoring system Relay contacts for alarm output (2 sets) Maximum load: 30 V DC, 1 A | | | |
| Power requirements | Supplied via power supply unit KZ-50 (90 V to 250 V AC, supplied power cord only for use in Japan, 100 V AC) | | | |
| Power consumption | Max. 40 VA (including power supply unit) | | | |


Ambient conditions for operation

| | $\begin{array}{c} 35 \\ 25 \\ 15 \\ 0 \\ 0 \\ 0 \\ 20 \\ 40 \\ 60 \\ 85 \\ Humidity (\%) \end{array}$ | | | |
|--------------------------------|--|---------------|--|--|
| Ambient conditions for storage | | | | |
| | -10° C to $+50^{\circ}$ C, 85% RH or less | | | |
| | (no condensation and no freezing in internal piping | g) | | |
| Dimensions and Weight | | | | |
| Main unit (KS-16F): | 124 mm (H) × 248 mm (W) × 193 mm (D) (Max.) | | | |
| | $110 \text{ mm} (\text{H}) \times 240 \text{ mm} (\text{W}) \times 150 \text{ mm} (\text{D}) (excluding the second s$ | ng protruding | | |
| | parts) | 01 0 | | |
| | Approx. 3.5 kg | | | |
| Power supply unit (KZ-50): | | | | |
| | 130 mm (H) \times 71 mm (W) \times 200 mm (D) (Max.) | | | |
| | 112 mm (H) \times 71 mm (W) \times 185 mm (D) (excluding | ng protruding | | |
| | parts) | | | |
| | Approx. 0.8 kg | | | |
| Supplied accessories | Tube A vacuum pack | 1 | | |
| | $(2 \text{ mm} \times 4 \text{ mm} \text{ dia.}, 1.5 \text{ m} \text{ flared PFA tube 2, unio})$ | | | |
| | Power cord (only for use in Japan, 100 V AC) | 1 | | |
| | DC cable | 1 | | |
| | Power supply unit KZ-50 | 1 | | |
| | Slow-blow fuse (2 A) | 1 | | |
| | Instruction manual | 1 | | |
| | Liquid-borne particle counter usage precautions | 1 | | |
| | Inspection certificate | 1 | | |
| | | | | |

Shaded section _____ in graph below (no condensation)

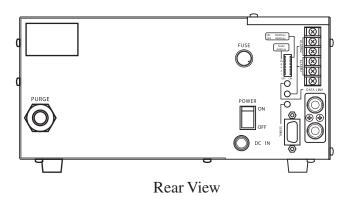

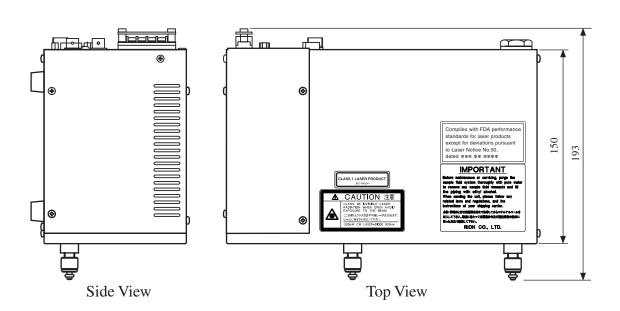


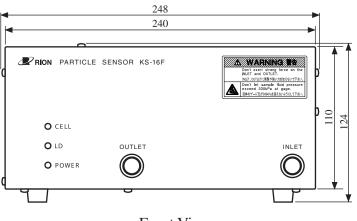

Front View

Unit: mm

Main unit (KS-16F) dimensions

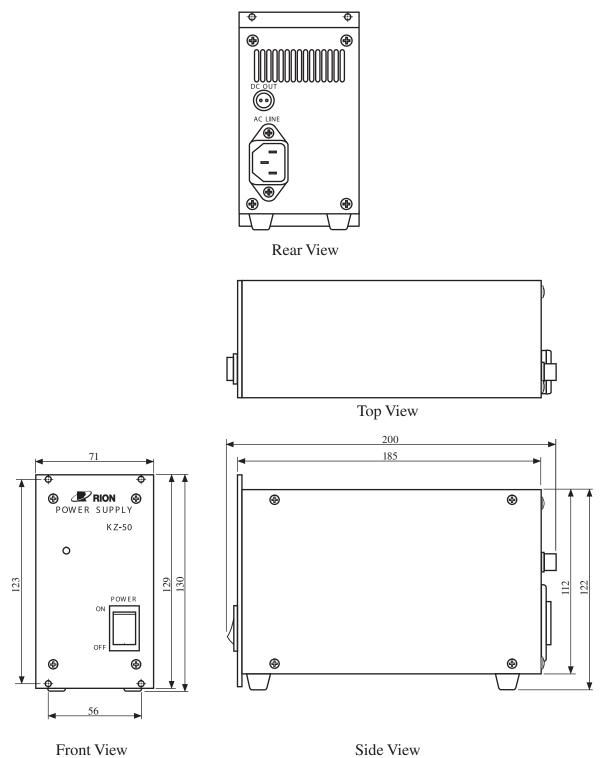

Side View

Unit: mm

Power supply unit (KZ-50) dimensions

Specifications subject to change without notice